
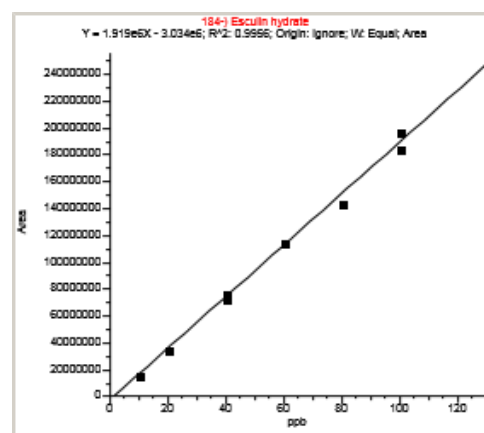
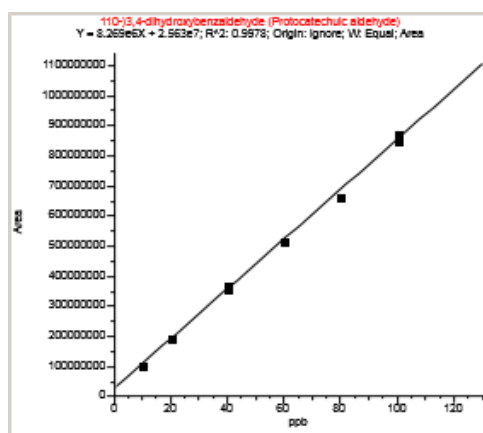
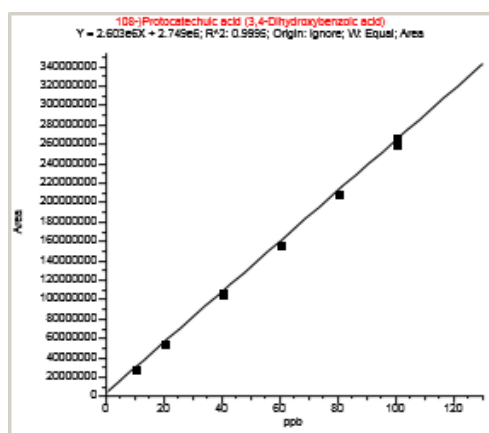
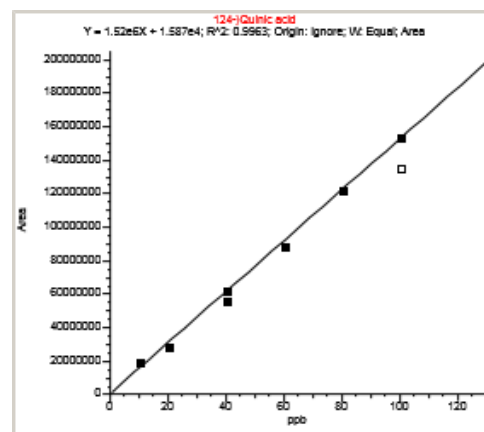
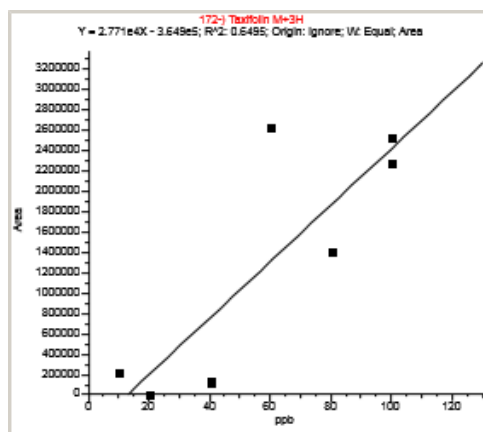
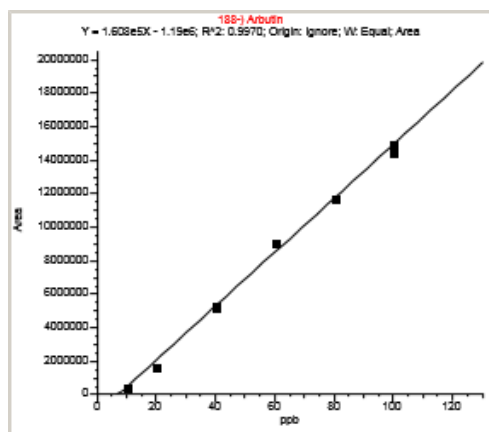
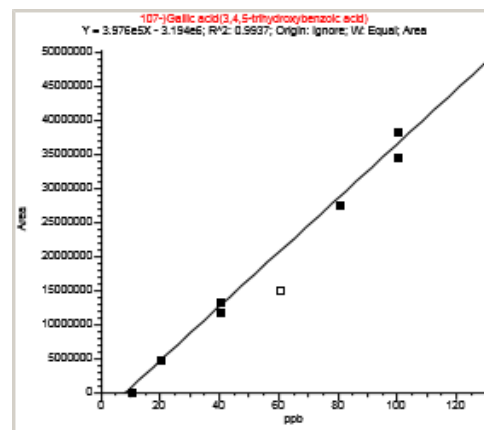
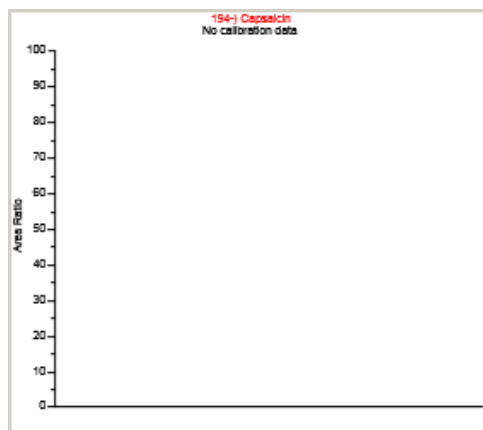


High Density Calibration Report

Lab Name: Default Laboratory
 Instrument: Thermo Scientific Instrument
 User: Thermo
 Batch: FENOLICQUAN-13










Method: FENOLICQUAN-13_FENILICQUAN
 FENILICQUAN
 Cali File: FENOLICQUAN-13.calx

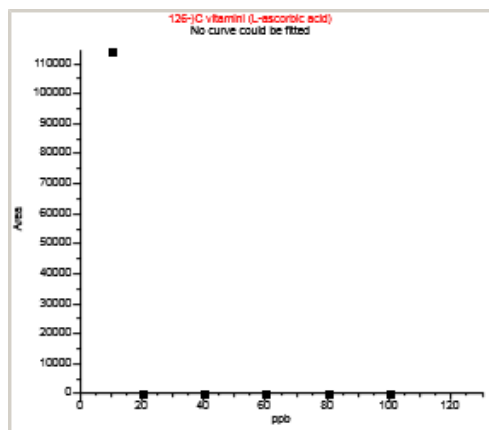

High Density Calibration Report

Lab Name: Default Laboratory
 Instrument: Thermo Scientific Instrument
 User: Thermo
 Batch: FENOLICQUAN-13










Method: FENOLICQUAN-13_FENOLICQUAN
 FENOLICQUAN
 Cali File: FENOLICQUAN-13.calx

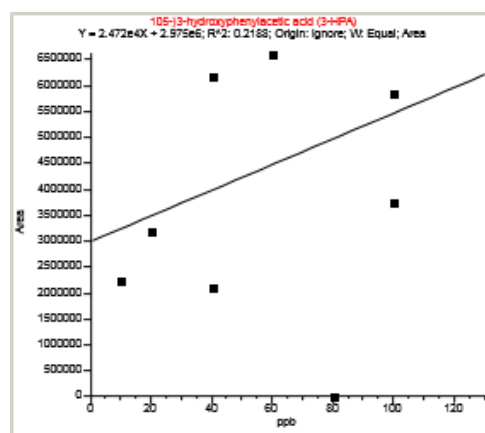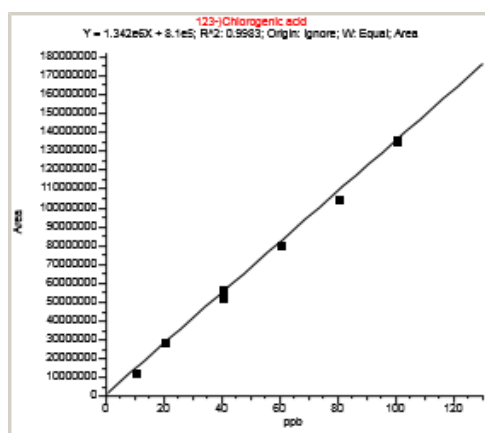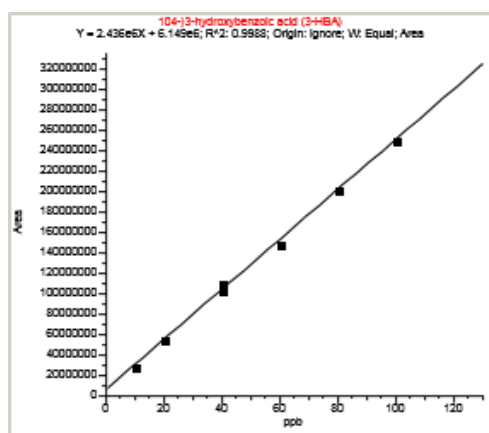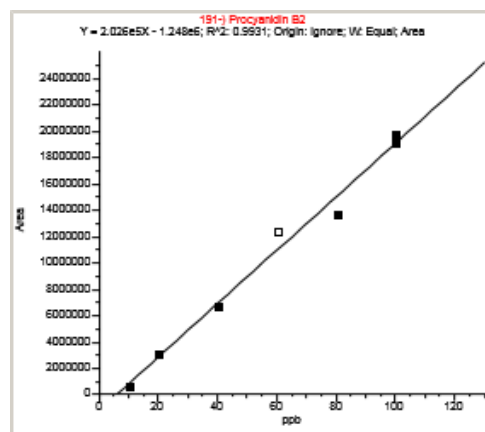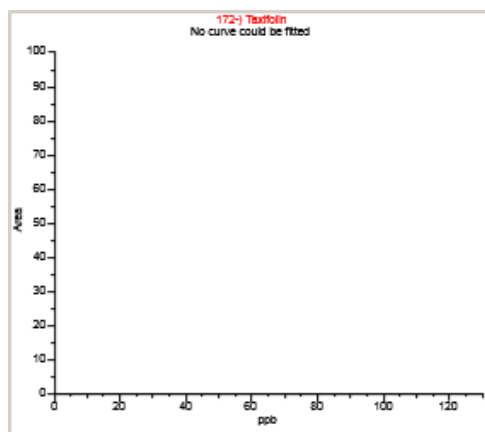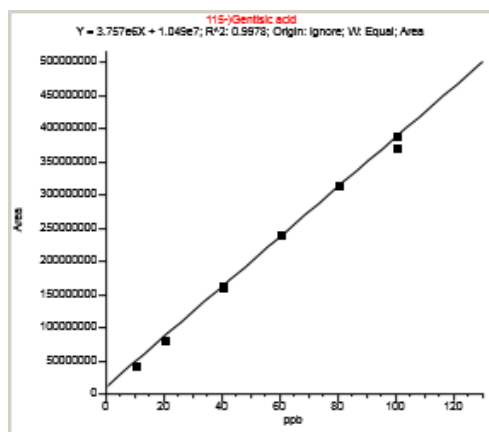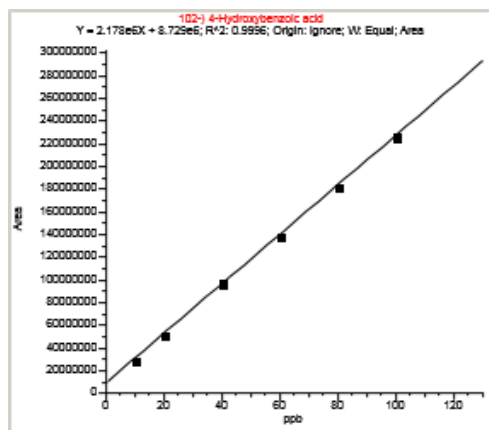

High Density Calibration Report

Lab Name: Default Laboratory
 Instrument: Thermo Scientific Instrument
 User: Thermo
 Batch: FENOLICQUAN-13










Method: FENOLICQUAN-13_FENOLICQUAN
 FENOLICQUAN
 Cali File: FENOLICQUAN-13.calx

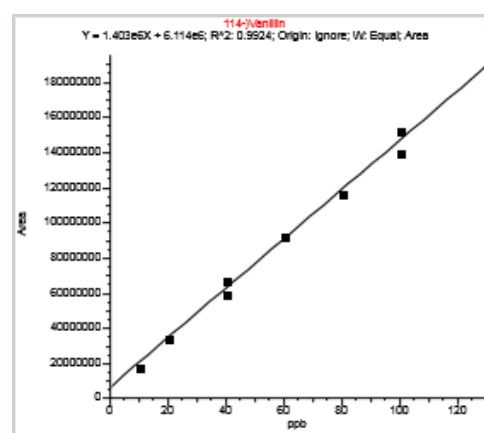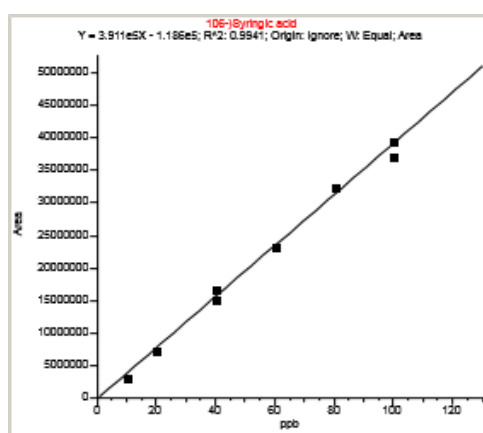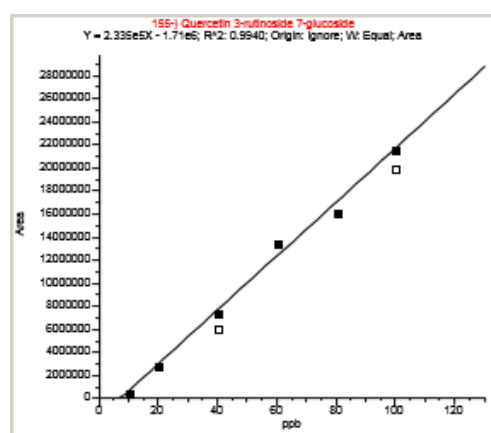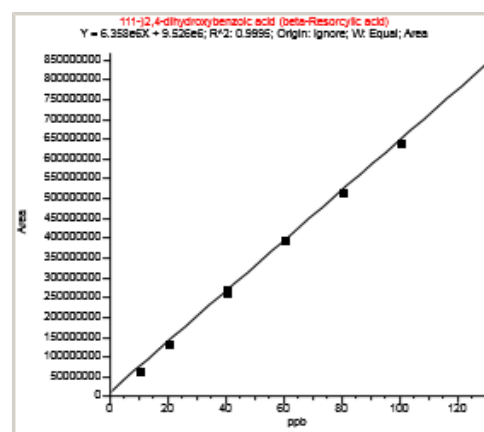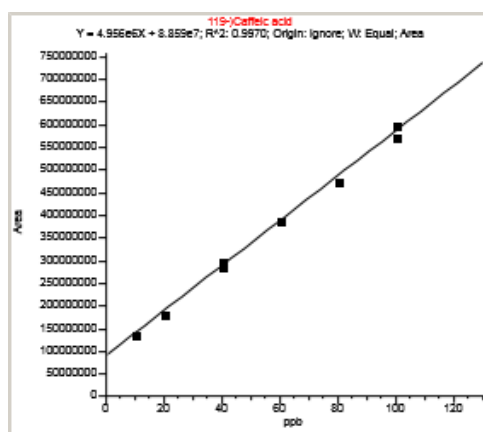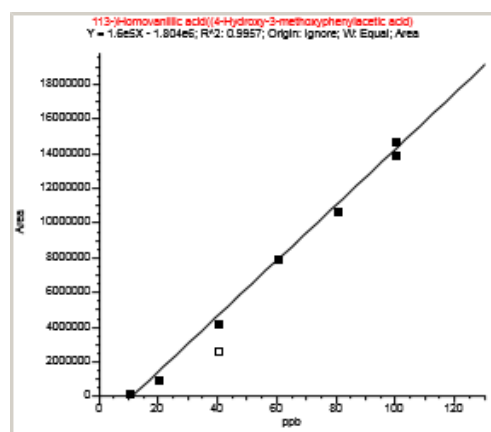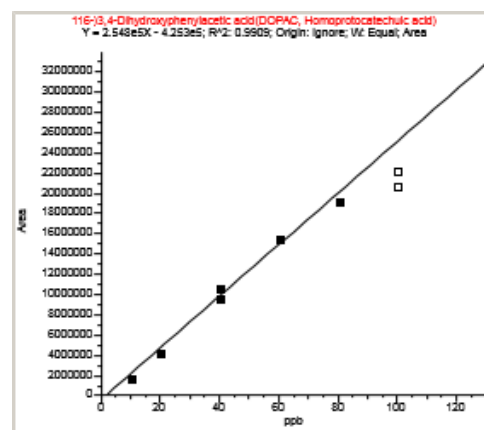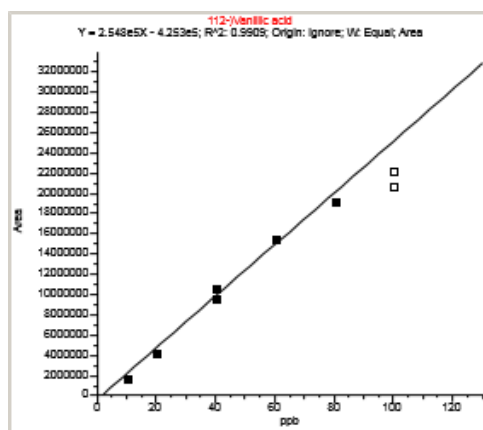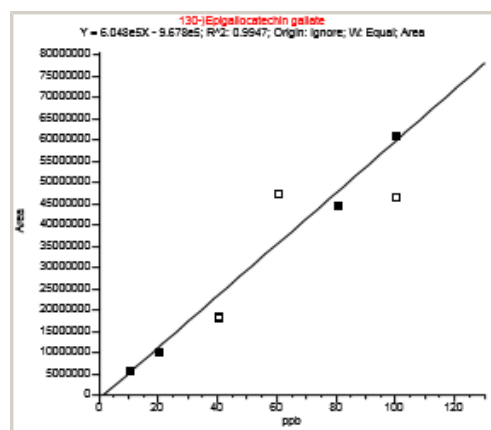

High Density Calibration Report

Lab Name: Default Laboratory
 Instrument: Thermo Scientific Instrument
 User: Thermo
 Batch: FENOLICQUAN-13










Method: FENOLICQUAN-13_FENOLICQUAN
 FENOLICQUAN
 Cali File: FENOLICQUAN-13.calx

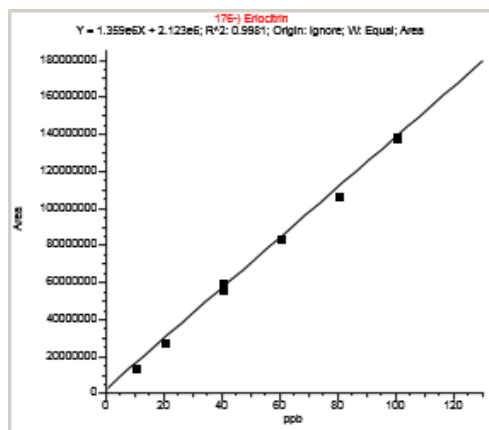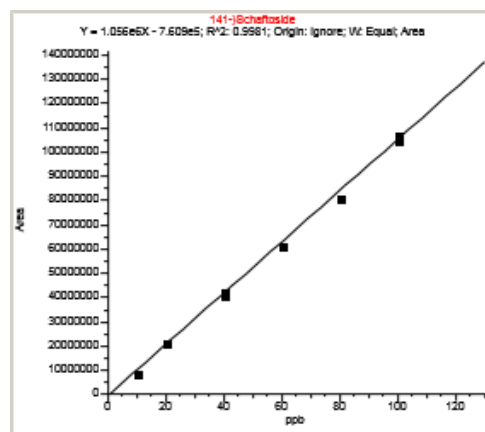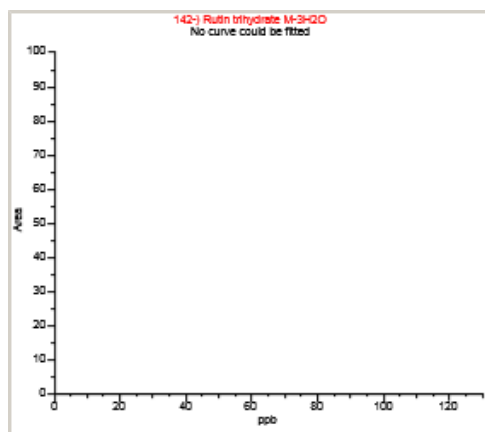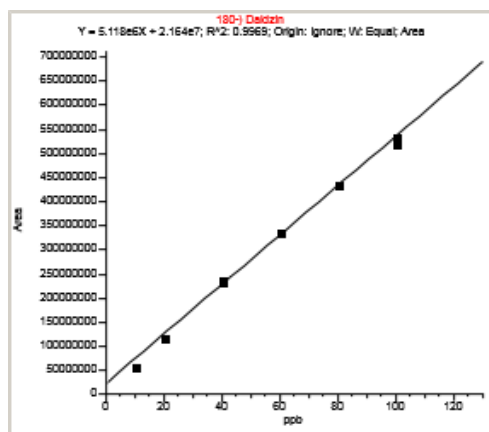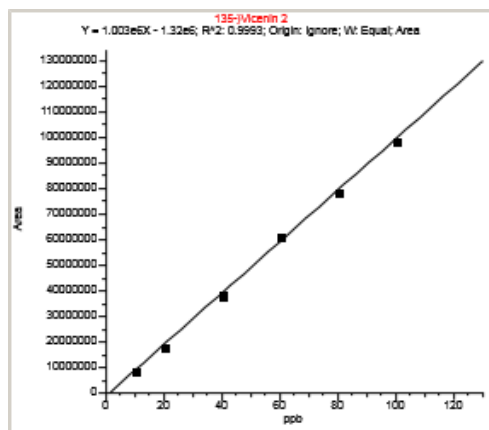

High Density Calibration Report

Lab Name: Default Laboratory
 Instrument: Thermo Scientific Instrument
 User: Thermo
 Batch: FENOLICQUAN-13










Method: FENOLICQUAN-13_FENILICQUAN
 FENILICQUAN
 Cali File: FENOLICQUAN-13.calx

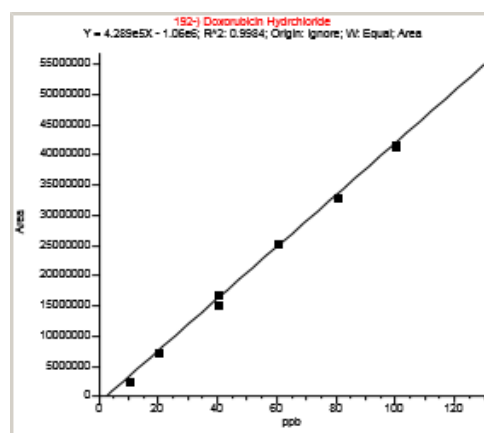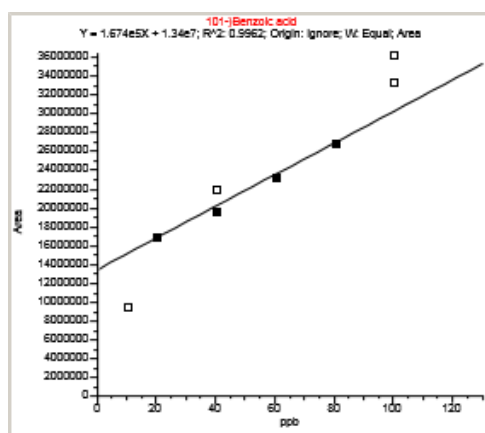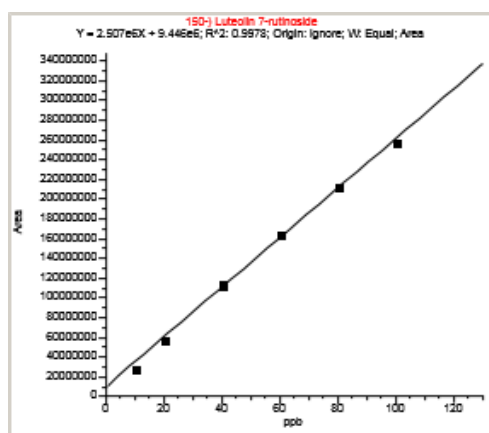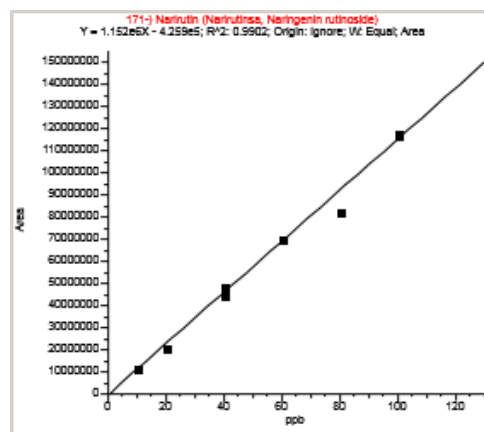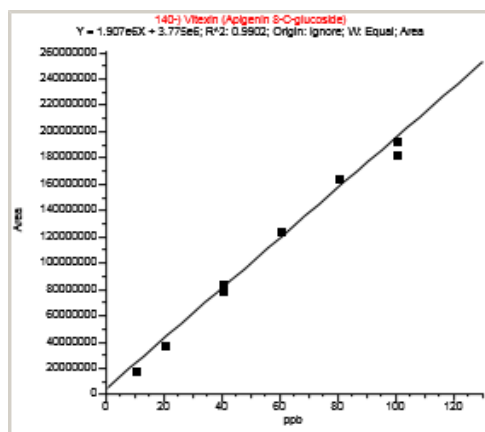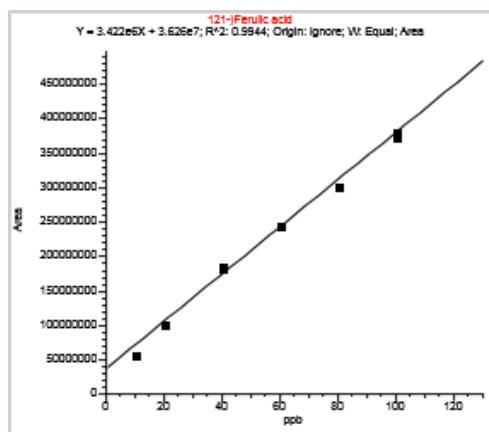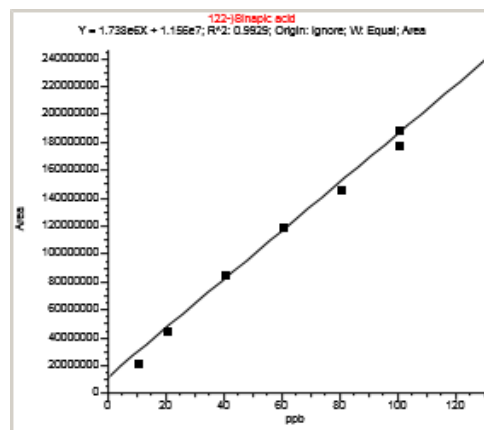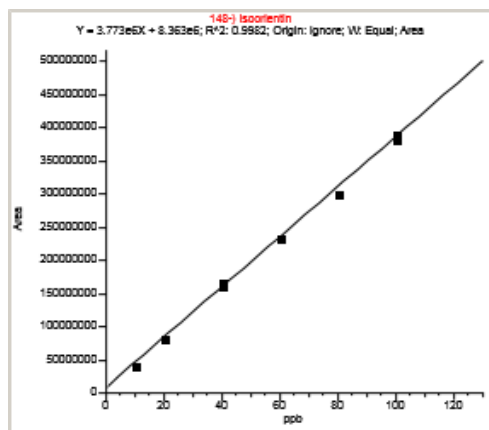

High Density Calibration Report

Lab Name: Default Laboratory
 Instrument: Thermo Scientific Instrument
 User: Thermo
 Batch: FENOLICQUAN-13










Method: FENOLICQUAN-13_FENILICQUAN
 FENILICQUAN
 Cali File: FENOLICQUAN-13.calx

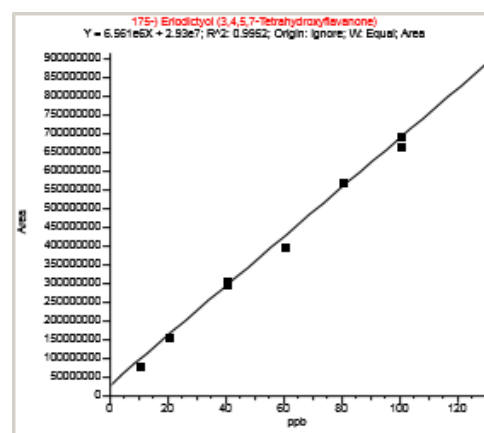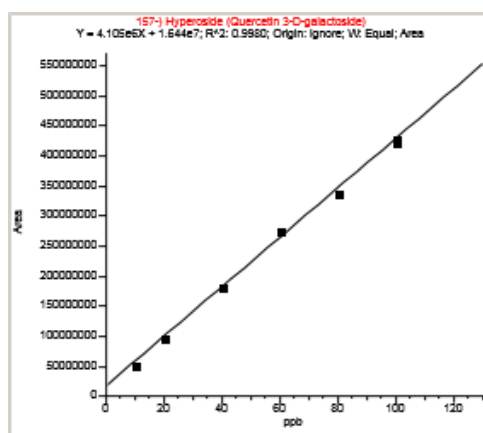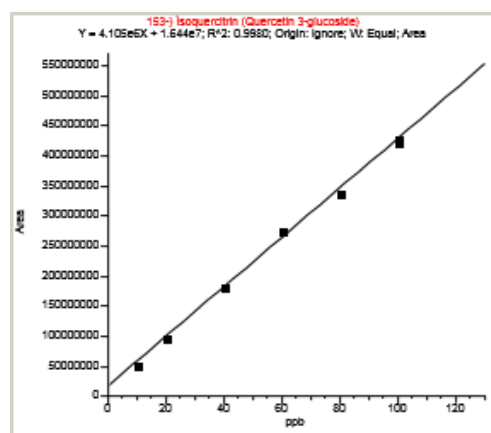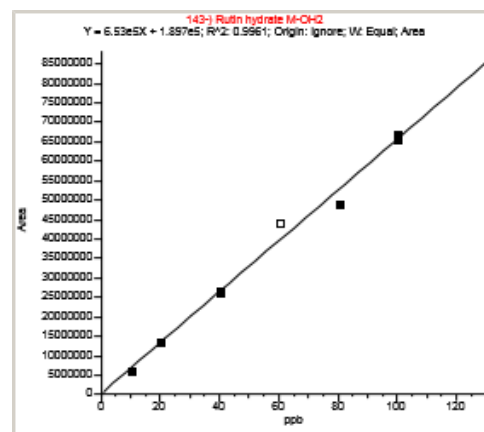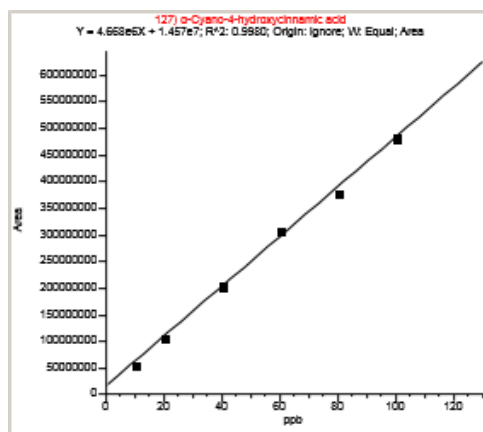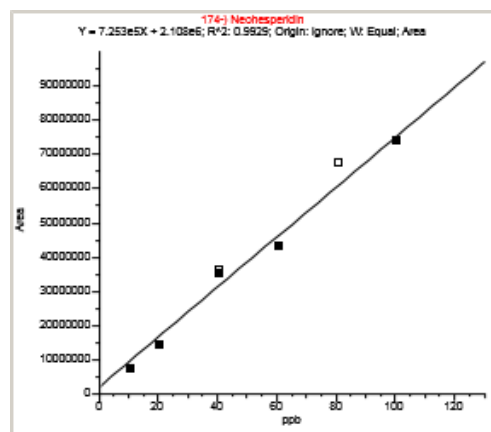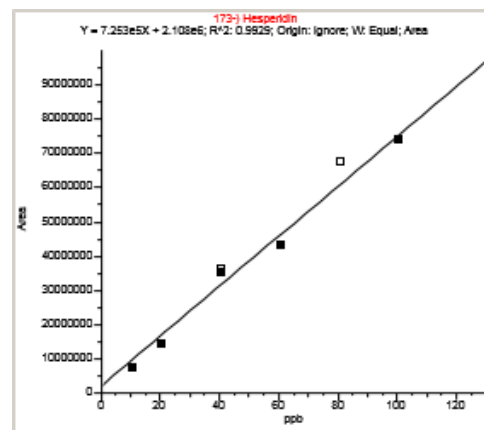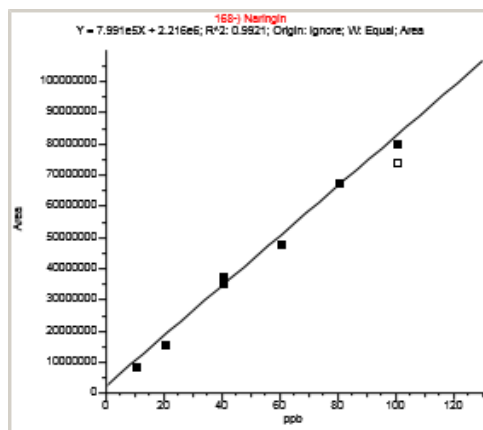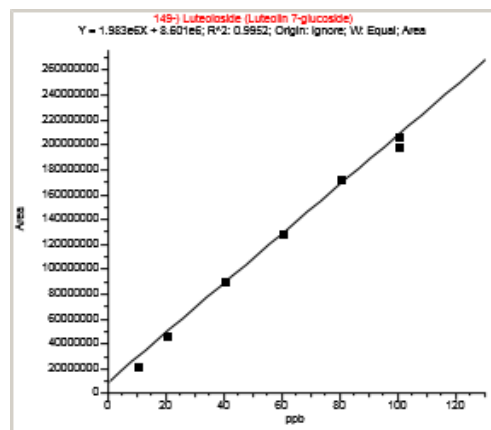

High Density Calibration Report

Lab Name: Default Laboratory
 Instrument: Thermo Scientific Instrument
 User: Thermo
 Batch: FENOLICQUAN-13










Method: FENOLICQUAN-13_FENOLICQUAN
 FENOLICQUAN
 Cali File: FENOLICQUAN-13.calx

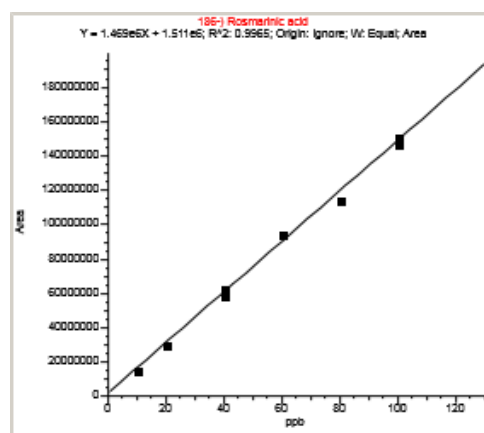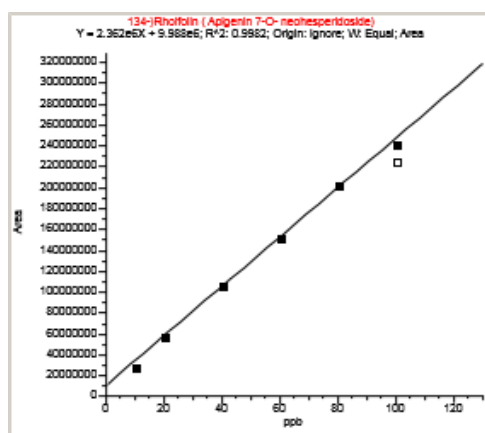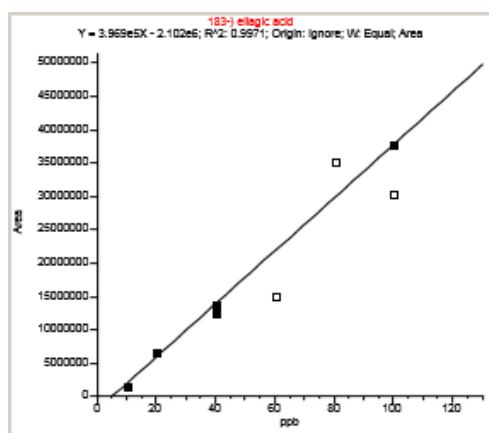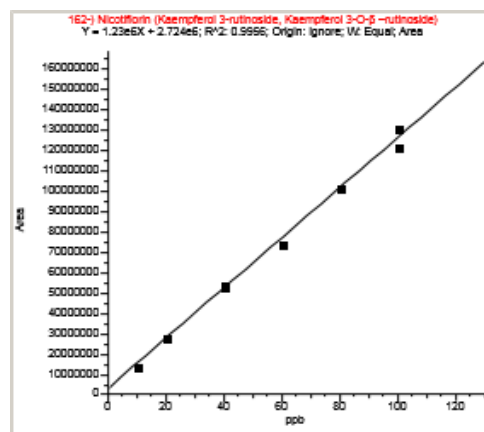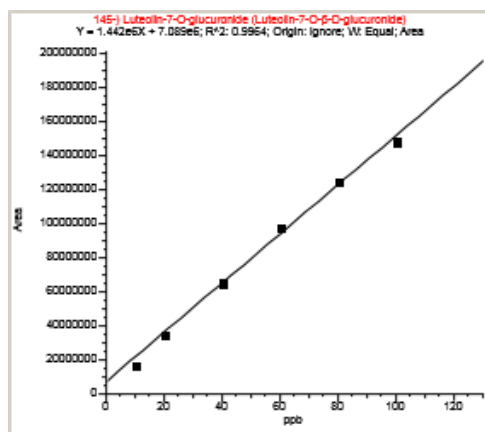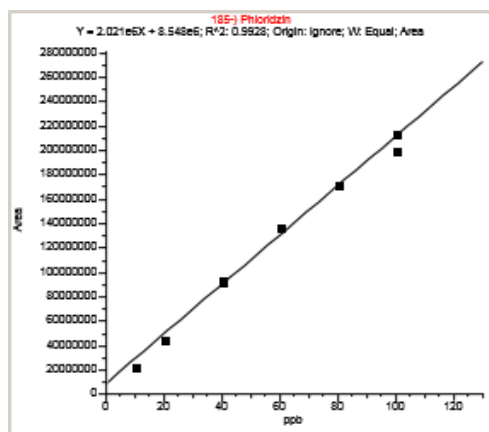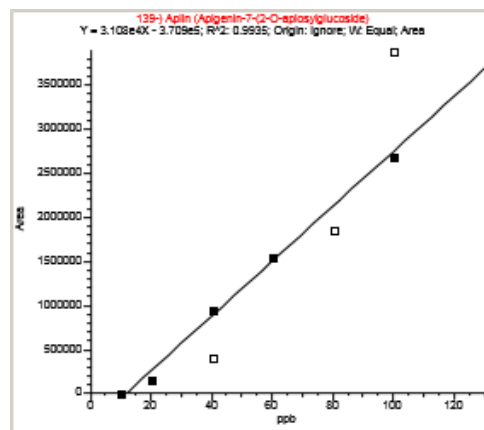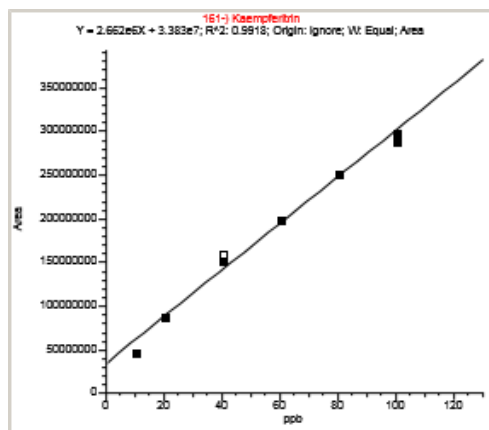

High Density Calibration Report

Lab Name: Default Laboratory
 Instrument: Thermo Scientific Instrument
 User: Thermo
 Batch: FENOLICQUAN-13










Method: FENOLICQUAN-13_FENILICQUAN
 FENILICQUAN
 Cali File: FENOLICQUAN-13.calx

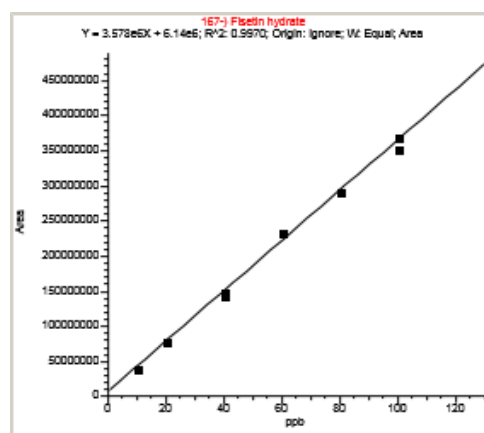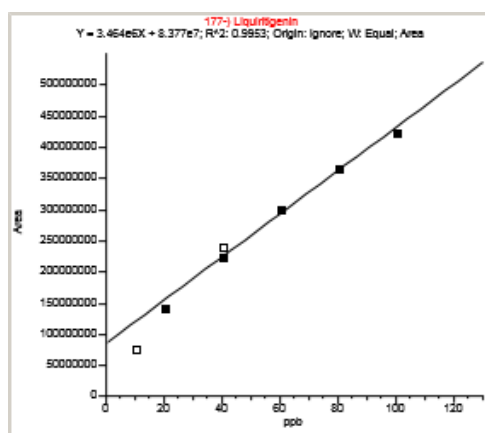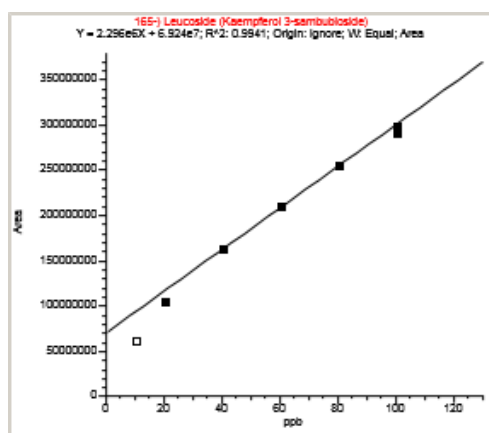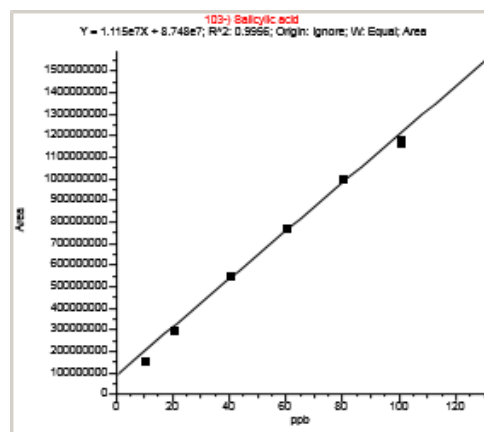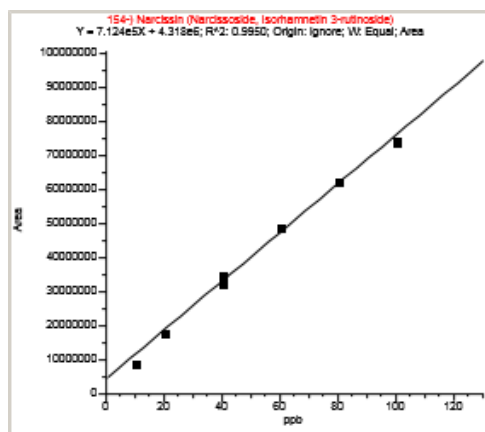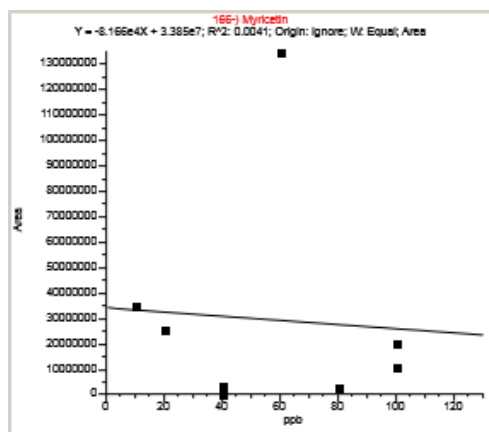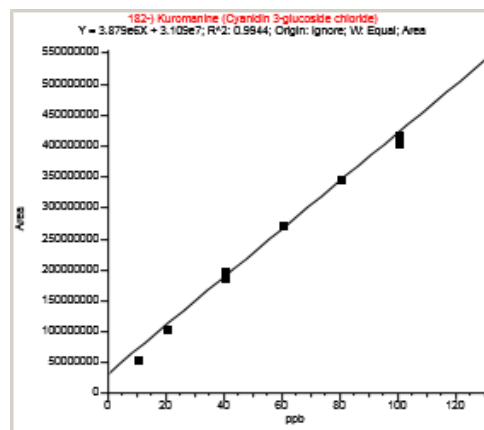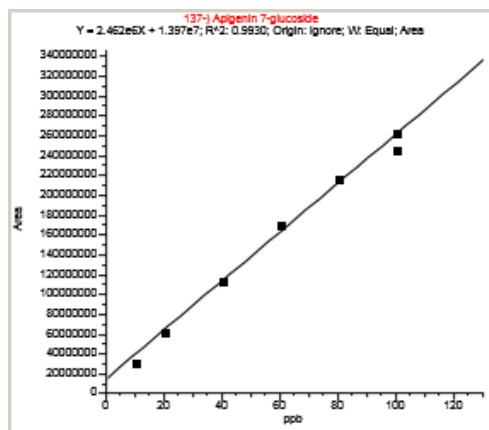

High Density Calibration Report

Lab Name: Default Laboratory
 Instrument: Thermo Scientific Instrument
 User: Thermo
 Batch: FENOLICQUAN-13










Method: FENOLICQUAN-13_FENOLICQUAN
 FENOLICQUAN
 Cali File: FENOLICQUAN-13.calx

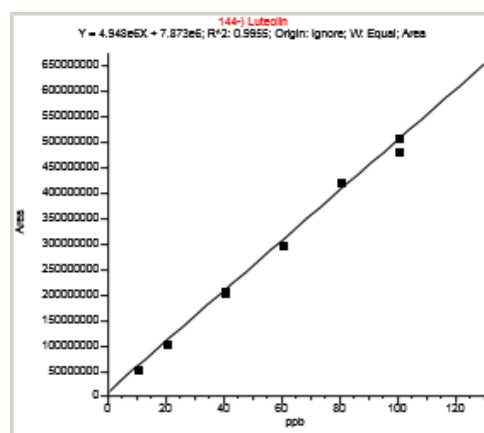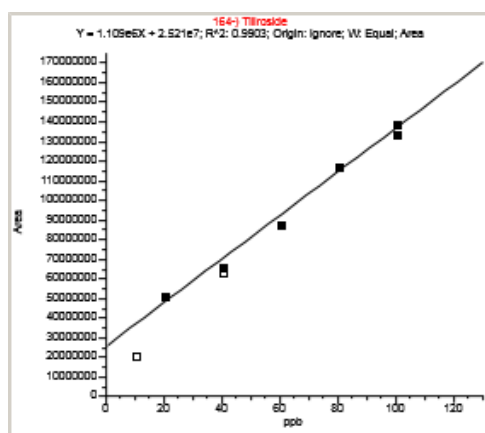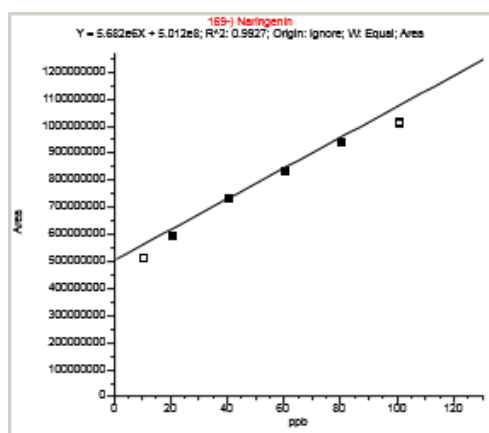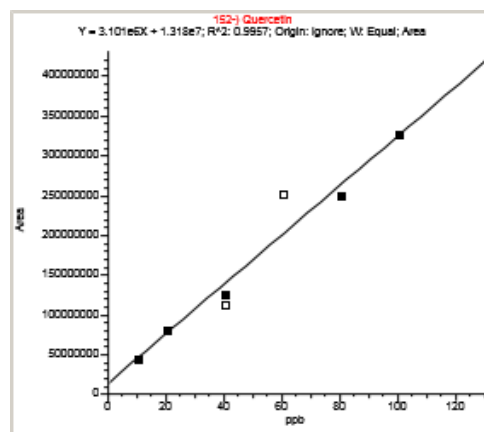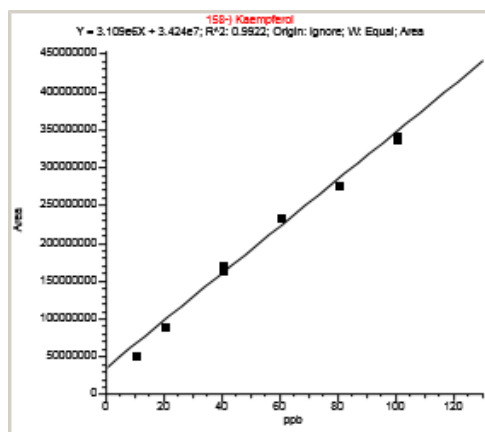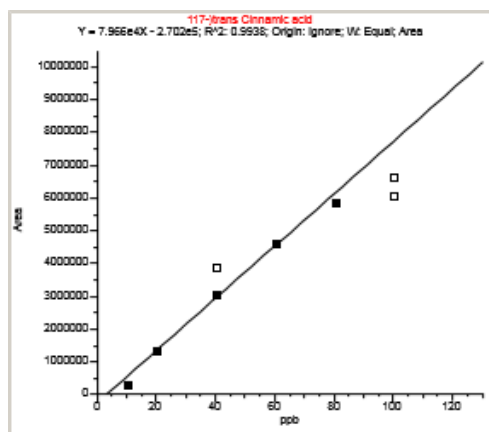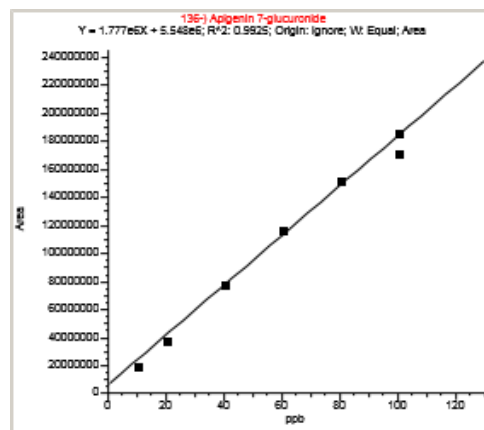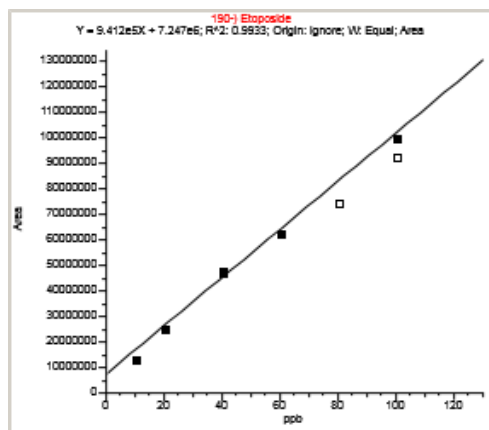

High Density Calibration Report

Lab Name: Default Laboratory
 Instrument: Thermo Scientific Instrument
 User: Thermo
 Batch: FENOLICQUAN-13

Method: FENOLICQUAN-13_FENOLICQUAN
 FENOLICQUAN
 Cali File: FENOLICQUAN-13.calx

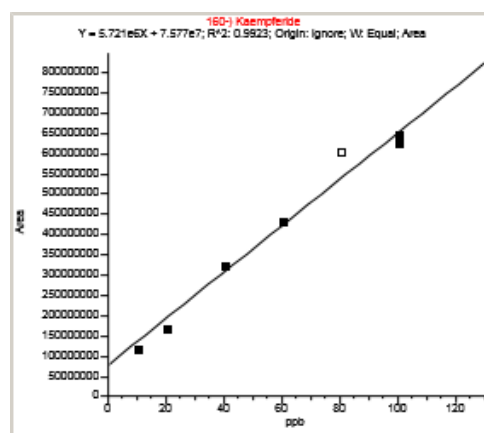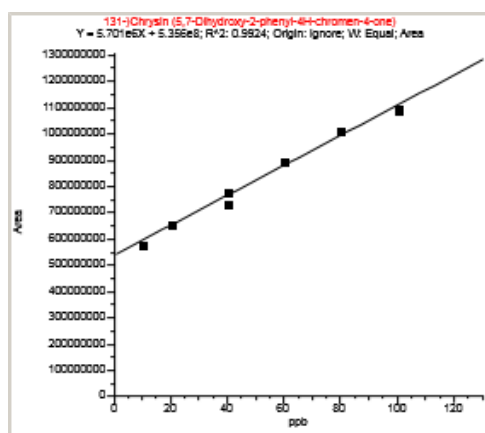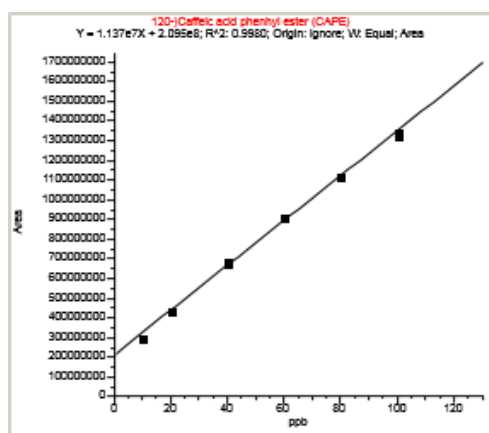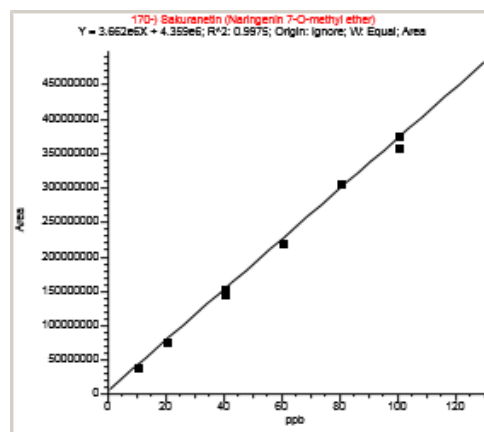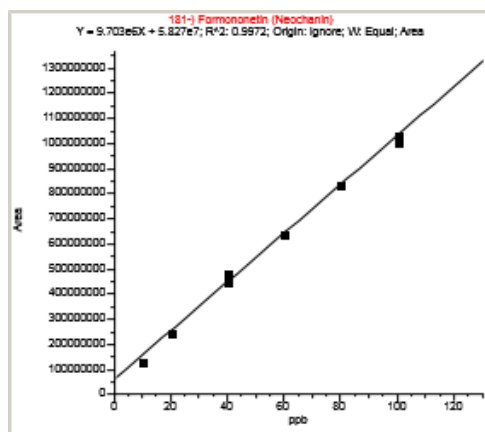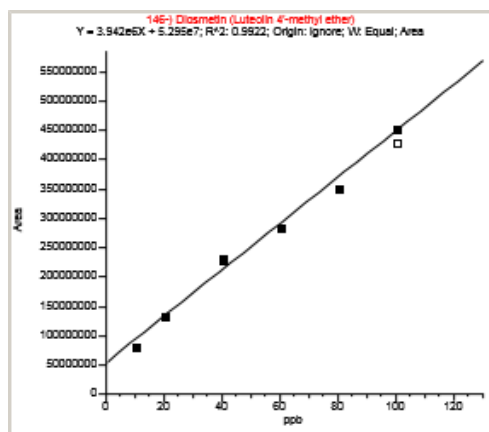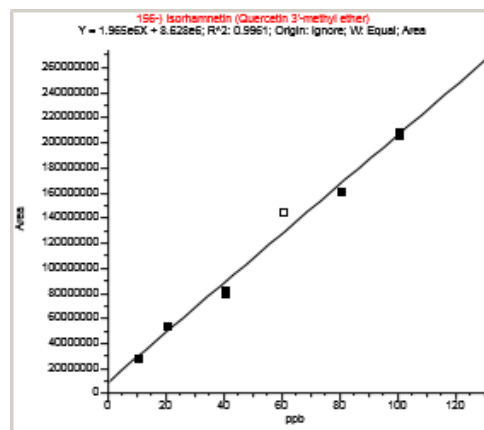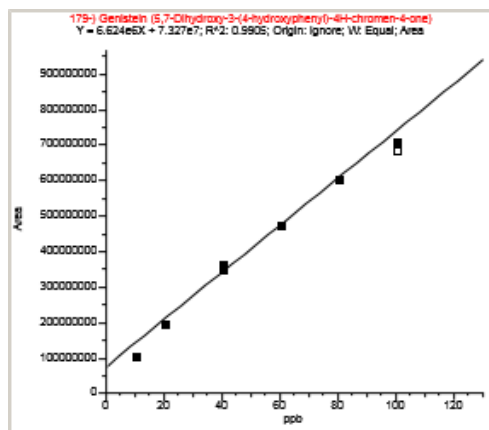

High Density Calibration Report

Lab Name: Default Laboratory
 Instrument: Thermo Scientific Instrument
 User: Thermo
 Batch: FENOLICQUAN-13

Method: FENOLICQUAN-13_FENILICQUAN
 FENILICQUAN
 Cali File: FENOLICQUAN-13.calx

